



Vicious circle in Zirconia Bonding: A Review

Dr Priyanka Somashekhar

Submitted: 01-01-2025

Accepted: 10-01-2025

ABSTRACT:

The preferred material for fixed dental restorations is zirconium dioxide ceramics because of their excellent mechanical and optical properties. However, these materials have a drawback in that they do not adhere well to natural tissues or synthetic substrates. Traditional adhesive techniques used with silica-based ceramics do not work effectively with zirconia. Currently, several technologies are being utilized clinically to overcome this problem, and other approaches are under investigation. (1) Most focus on surface modification of the inert surfaces of high strength ceramics. The ability to chemically functionalize the surface of zirconia appears to be critical in achieving adhesive bonding. This article discusses the current options and newer technologies being developed to address this issue.

Key words: Zirconium dioxide ceramics; Adhesion; Bonding; Surface Modification; Surface Functionalization; Zirconia


I. INTRODUCTION:

The growing belief that metal-free dentistry will alter the traditional restorative spectrum has been stymied by the brittle nature of the ceramics. Therefore, they have been developed Y-TZP commonly known as "ZIRCONIA" (2). The emergence of zirconia alongside CAD/CAM technology has allowed the field of dental science to realize its aspirations. (3) This zirconia contains 3 mol% of yttria (Y_2O_3) as a stabilizer. Compared to all other ceramic core materials, Zirconia has exceptional flexural strength (900-1000 MPa) and fracture toughness (5.5 - 7.4 MPa-m^{1/2}), resulting in a highly fracture resistant material. [1]. However, several problems arise because of its high surface stability, particularly with regard to the effectiveness and longevity of the chemical or mechanical bond with the various cementing systems. Due to zirconia's high acid resistance and the lack of a glassy matrix on which these substances act, the common etching methods with hydrofluoric acid and silanization techniques that were previously employed for other ceramic systems have not been worked well against it [2]. Unfortunately, the composition and physical

properties of ZrO_2 differ from traditional silica-based materials such as porcelain. Zirconia is not easily etched by HF and requires very aggressive mechanical abrasion methods to increase surface roughness, potentially leading to strength-reducing surface defects [3-5]. In this article we discuss: (1) Zirconia as a bioceramic material (2) Chemico-Mechanical coupling bond (3) zirconia and CAD/CAM Dentistry (4) The bond between zirconia and veneering ceramics, (5) The bonding of zirconia with resin based luting cements, (6) Enamel wear against polished and glazed zirconia restoration and (7) Evaluation of clinical efficacy on zirconia restoration.

1. Zirconia as a bioceramic material


In 1789, The German chemist Martin Heinrich Klaproth discovered zirconium oxide (ZrO_2), commonly referred to as zirconia, as a reaction produced by heating a gem called zircon [6]. The term Zirconium is coming from the Arabic Zargon 14 (golden) and the Persian terms Zar (gold) and Gun (colour). Zr is a white metal (atomic number 40) with a density of 6.51.

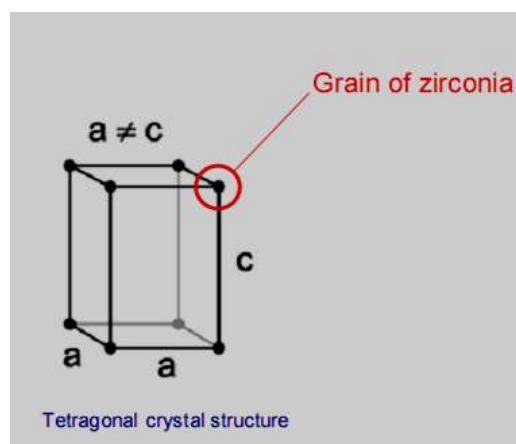

Zirconia is polymorphic, implying that it has a distinctive equiatomic (stable) crystal structure at varying temperatures while maintaining the same chemical form. There are three crystalline forms of it: monoclinic at lower temperatures, tetragonal at 1170 °C, and cubic at 2370 °C [7,8]. After cooling, the crystal structure of the material changes from a tetragonal crystal to a monoclinic crystal. This



causes a 3-4% increase in the volume of the material, which can lead to significant stresses. These stresses can lead to the formation of cracks, which in turn can lead to sagging, crumpling and failure. Ruff et al. discovered that by incorporating a small quantity of calcium, the cubic phase of ZrO₂ could be stabilized, enabling its utilization as an engineering material.

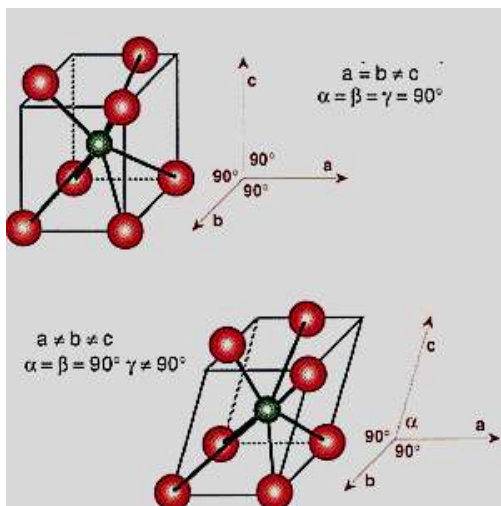

Over the years, other metal oxides like cerium oxide (CeO₂), magnesia (MgO), and yttria (Y₂O₃) have been used to create a range of partially stabilized zirconia (PSZ) compositions, which are primarily cubic phase at room temperature, with monoclinic and tetragonal precipitates as a minor phase [7]. PSZ is of particular interest because of its transformation toughening properties [9]. When a crack begins and spreads in a partially stabilized zirconia material under external force, the tetragonal phase near the crack tip can convert into a monoclinic phase repeatedly. The subsequent volume expansion from the transformation produces a compressive stresses near the crack tip. ZrO₂ was recently introduced into dentistry for its superior aesthetic potential in comparison to metal-ceramic structures. Zirconia is being investigated as a dental material for various clinical applications, such as brackets for orthodontic treatments [10], endodontic posts and dowels [11,12], abutments [13,14], single crowns [15] and fixed partial dentures [16]. Bonding to ZrO₂ has become an increasingly common problem in recent years. As already mentioned, typical adhesive bonds on ZrO₂ surfaces are ineffective due to their non-polar and inert properties. Additionally, hydrofluoric acid etchants do not provide sufficient surface roughness for easy micromechanical

adhesion. The process involves using Al₂O₃ particles to abrade the surface, then applying a tribosilica coating that allows for the formation of chemical bonds with a silane coupling agent and resin cement. This is a complicated method that does not provide bond strengths comparable with those observed for silane-bonded porcelain. [4,17,18]. There is concern that using air particle abrasion on ZrO₂

ceramics could cause microfractures, weakening them and potentially causing them to fail unexpectedly. The current methods for bonding ZrO₂ ceramics are not suitable for all medical uses, and it is unclear how long they will last.

2 Chemico-Mechanical coupling bond

A resilient bond is necessary to securely attach ZrO₂ to teeth or other surfaces. Mechanical bonding via micromechanical interlocking from surface roughening and, if feasible, chemical bonding between ceramic and cement are essential for resin bonding success. For surface roughening silica-based ceramics, phosphoric acid (H₃PO₄) or hydrofluoric acid (HF) etching are frequently suggested techniques [75]. This produces a clean, rough surface that increases surface area available for mechanical interlocking and enhances wettability. It is challenging to roughen the surface for mechanical retention on nonsilica-based ceramics, such as ZrO₂, due to the ineffectiveness of H₃PO₄ and HF. Because of the difficulty in creating mechanical and chemical bonding in ZrO₂, alternative methods have been explored to bond ZrO₂ using resins. Surface grinding is a commonly used alternative for roughening the surface of ZrO₂ to improve mechanical bonding. Surface grinding can be done in a number of ways, including with a diamond bur [20], particle air-abrasion with Al₂O₃ or other abrasive particles that range in size from 50 to 250 μm [19–20], and abrasive paper or wheels (SiCor Al₂O₃). Selective infiltration etching (SIE) is a new surface roughening method that has been investigated for ZrO₂. This uses a heat-induced maturation process to pre-stress surface grain boundaries in ZrO₂ to allow infiltration of boundaries with molten glass. The glass is then etched out using HF, creating a 3D network of inter-granular porosity that allows nano-mechanical interlocking of resin cement. The impact of treatments on the mechanical properties of ZrO₂ materials is debated, with both positive and negative results being reported [21–22]. Additionally, particle abrasion can lead to a



sharp cracks and structural defects, making zirconia more prone to radial cracking during use[23].

Organo-silanes, generally referred to simply as “silanes” in dentistry, are compounds that contain a silicon (Si) atom or atoms, are similar to orthoesters in structure, and display dual reactivity. One end of a silane molecule is organically functional (e.g., vinyl-CH₂, amino-NH₂), and can polymerize with an organic matrix (e.g., a methacrylate). The other end is generally comprised of alkoxy groups (e.g., methoxy-OCH₃, ethoxy-OCH₂CH₃), which can react with a hydroxylated surface, like porcelain. Due to the lack of silica in ZrO₂, silica-coating techniques have been explored to utilize the chemical bonding provided by silanization. Experimentation with different silane coupling agents has resulted in enhancement of luting of ZrO₂. Matinlinna et al. [24] researched use of three trialkoxysilanes, 3-methacryloyloxypropyltrimethoxysilane (MPS), 3-acryloyloxypropyltrimethoxysilane (ACPS), and 3-isocyanatopropyltriethoxysilane (ICS), in enhancing the bonding of two resin cements, an experimental Bis-GMA and commercial Bis-GMA (RelyX ARC, 3M ESPE, Seefeld, Germany), to ZrO₂. They determined that application of a tribochemical coating, followed by silanization with MPS and ACPS, were successful in bonding the two cements to ZrO₂. Recent advancements in silicoating technology, specifically the Pyrosil Pen Technology (Pyrosil Pen, Sura, Instruments, Jena, Germany), have made it easier to use in dental procedures. However, research has shown that there is no significant difference in bond strength between different types of ceramics. ZrO₂-based ceramics have been found to have a lower bond strength compared to silicoated silica and alumina-based ceramics. This could be attributed to the fact that the ceramic surface was only ground using 800 grit grinding paper, resulting in a lack of micromechanical bonding [24].


3. Zirconia and CAD/CAM Dentistry.

Zirconia-based ceramics, specifically Y-TZP, are a viable alternative to metal frameworks for dental prostheses[25,26]. Y-TZP frameworks can be made by milling a solid block using CAD/CAM

procedures through two different systems.

The first system allows for milling directly from fully sintered ceramic blocks, resulting in a better fit but with the drawback of tool wear. The second system involves milling from partially-sintered or green blocks, followed by post-sintering at high temperature to strengthen the framework. This system is currently popular for fabricating zirconia frameworks using the main CAD/CAM systems available in the world market. Although this technique has the advantage of easy machinability without tool wear and chipping of the material, the dimensions of the frameworks need to be adjusted to allow for compensating sintering shrinkage during the post-sintering process to ensure the finished frameworks fit well. The clinical evaluation found that the fit of zirconia-

ceramic fixed dental prostheses (FDPs) made with CAD/CAM systems was similar to conventional metal ceramic restorations [25]. However, for FDPs with 3-unit and 4-unit frameworks, the shrinkage of the pontic part caused a bigger difference in the fit of the crown next to the pontic. Therefore, when using partially-sintered or green blocks, we need to be careful about the distortion of zirconia-based FDPs with longer spans[26]. The procedures used to fabricate CAD-CAM FDPs are shown in **Fig. 1**. An intraoral digitizer scanned the intraoral abutment in order to generate an optical impression. The monitor displayed reconstructed digital data as three-dimensional visuals, and it was used to virtually build the ideal FDP morphology. A numerically controlled machine was used to grind a block in order to fabricate real FDPs.

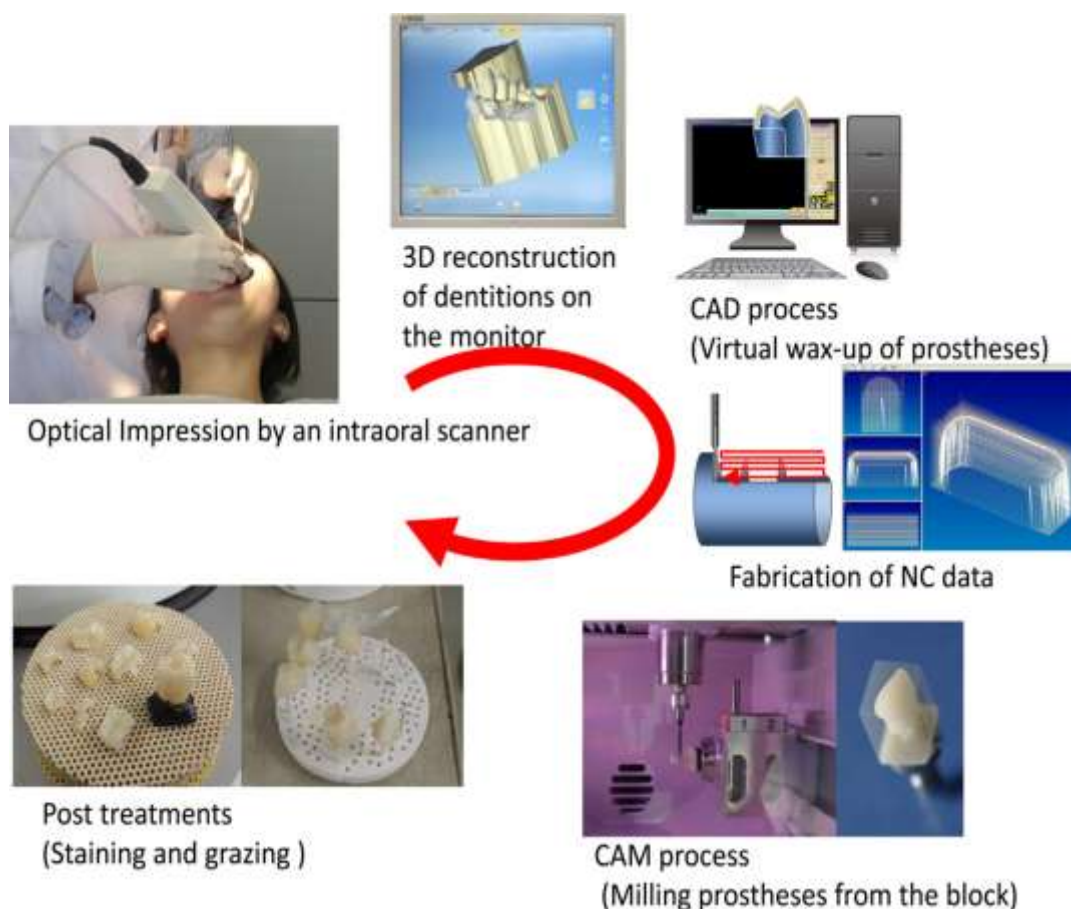

4. The bond at zirconia / veneering ceramics

One of the specialized ways of using zirconia in dentistry is to fabricate zirconia frames upon which tooth-colored veneering ceramic is bonded. At present, there are two widely used methods of securing ceramic onto zirconia frames: the layering technique and the press technique. In the layering technique, porcelain powder is applied onto the zirconia frame before firing. In the press technique, the lost wax technique is used to create the restoration. Homogeneous ceramic ingot is heated and then forced under pressure into a wax formed void. For both the layering technique and the press technique, the coefficient of thermal expansion of the veneering ceramic is set to be the same as or slightly lower than that of zirconia. This is because a large difference in the coefficient of thermal expansion between a zirconia frame and veneering ceramic will cause residual stress on the crown, thus resulting in reduced reliability of the restoration. There are some studies comparing the layering technique with the press technique, however, many reports argue that the dislodgement or fracture of veneered ceramics is more affected by frame design than differences in molding techniques [26-28]. The integration of metal and

porcelain in PFM crowns involves both mechanical and chemical bonding. However, there is not enough evidence to prove the presence of chemical bonding between zirconia and veneering ceramics, although there is one study[29] suggesting it. Therefore, it is believed that mechanical bonding is the main factor in the integration of zirconia-based restorations. A standard (ISO9693) exists for evaluating the bond strength between metal and porcelain through a bending test, and PFM restorations used in clinical practice should have a bond strength of 25 MPa or higher.[30]. Although there have not been many reports [31-33] concerning the evaluation of zirconia-to-porcelain integration using a bending test (ISO9693), all of those reported that the bond strength was 25 MPa or more. The bonding process between zirconia and veneering ceramics in dentistry still has many unanswered questions about how it works. Further research and the development of a dependable clinical procedure will be needed in the future.



5. Bond of zirconia with resin-based luting cements:

In order to obtain the strong bond to zirconia ceramics in clinical conditions, it is important for the bonding surface to be roughened, activated for chemical bonding and free of any contaminants. The most commonly used material to attach a ceramic prosthesis to teeth is resin-based composite cement. However, it is difficult to bond ZrO₂ (a type of ceramic) to teeth using traditional resin composite cements because it does not contain silica. Previous studies [34] have shown that a resin-based composite cement containing phosphate monomer (7) can create a strong bond with alumina, but Bis-GMA (another type of resin) cannot bond with particle air-abraded alumina. The long-term bond strength of resin-based composite cements with phosphate monomer and ZrO₂ was first reported by Kern and Wegner [35]. Methods for chemically altering the surface of zirconia using silicon compounds and then applying silane monomers have been presented. Janda et al. [36] compared bonding performance of silica, alumina, and two zirconia ceramic materials treated with a flame treatment and silane priming. Although the flame treatment was successful for all ceramic materials, the results showed that the silica and alumina ceramics had stronger bond strengths than the zirconia ceramic materials. According to reports, the use of silica coating, silane, and MDP together is currently considered one of the most dependable bonding systems for zirconia [37-40]. Tanaka et al. [40] found that a strong bond was formed on Rocatec-coated Katana zirconia when a phosphate monomer and silane were used together. This was confirmed through X-ray photoelectron spectroscopy analysis. This bonding mechanism is substantially the same mechanism as bonding to feldspathic porcelain with silane/MDP bonding agent. In a study by Nakayama et al. [41], the bonding between a zirconia material and tri-n-butylborane (TBB) initiated luting agent was evaluated using different primers. The researchers found that using either the Alloy Primer or the Estenia Opaque Primer, both of which contain MDP, resulted in strong and long-lasting bonding between the zirconia and the TBB-initiated luting agent.

6. Enamel wear against polished and glazed zirconia restoration:

Different types of ceramics have been used in dentistry for restorative purposes. Zirconia is considered the best material in terms of strength and physical properties. However, when used for aesthetically pleasing dental restorations like crowns and bridges, zirconia is typically covered with feldspathic porcelain because it lacks sufficient translucency. Unfortunately, the porcelain veneer alone is not strong enough to serve as a dental restoration, particularly for posterior teeth. This has led to instances of clinical failure, with most cases attributed to porcelain chipping [42,43]. A new type of zirconia called high translucent zirconia has been introduced in dentistry [44,45]. It can be used for full contour restorations without the need for a covering porcelain, meaning that the zirconia surface is exposed to the mouth. The wear of opposing teeth is a significant concern. Dentists use mirror polishing to prevent wear on the enamel that opposes zirconia restorations (8). However, there is a misconception that antagonist enamel is easily worn due to its hardness (9). Additionally, it is unclear if glazing zirconia effectively prevents wear on opposing teeth. Recent studies have raised concerns about the wear of veneering porcelains on the opposing teeth. However, research has indicated that zirconia restoration with a proper surface polish causes the least amount of wear on the opposing enamel when compared to other dental materials.

These findings suggest that the wear of dental enamel caused by opposing surfaces is significantly influenced by the level of surface smoothness. **Figure 2** displays the roughness of three different types of dental zirconia after undergoing various grinding and polishing techniques [45]. Super Course, Sinter Dia, Vitreified Dia, and Ceram Dia M, F, and SF are rotary instruments used for grinding. Super Course, Sinter Dia, and Vitreified Dia exhibited high levels of roughness, exceeding 1 mm. However, Ceram Dia M, F, and SF had relatively low roughness, possibly due to the use of diamond grains fixed with artificial rubber. After grinding with Ceram Dia M, F, and SF, polishing was conducted using diamond pastes such as Diapolisher paste, Direct Dia paste, Zircon-Brite, and Zirkopol. The surface of the zirconia was made smoother by polishing, and the type of zirconia and diamond polishing paste used did not make a difference. Different cleaning pastes like ConCool, Pressage, and PTC regularly used in professional mechanical teeth cleaning (PMT) did



not affect the surface roughness when used after a specific polishing paste like Direct Dia . Fig 3 shows the glossiness of the same specimens increased at 60 degrees as the size of the diamond grains used in grinding instruments decreased, and further increased with additional polishing. However, the cleaning pastes used in professional mechanical teeth cleaning (PMTC)(50) did not cause any significant changes. This suggests that the

cleaning process does not interfere with maintaining proper oral hygiene when zirconia restoratives are used.

Fig. 4 shows the correlation between the glossiness and the surface roughness. The glossiness increased steeply with decreasing roughness to less than 0.3 mm. It suggests whether or not the final polishing is sufficient determines the final gloss of zirconia restoratives.

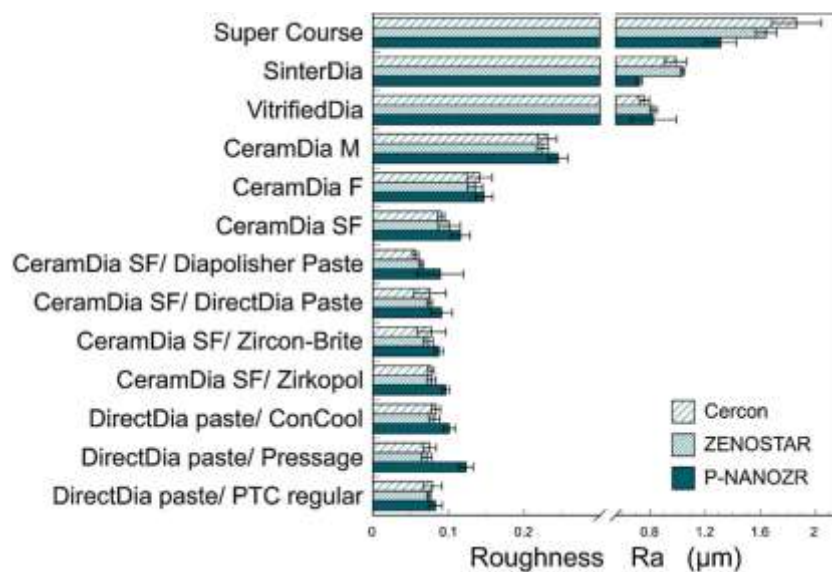


Fig 2: Surface roughness of three types of dental zirconia finished with 13 types of grinding and polishing condition

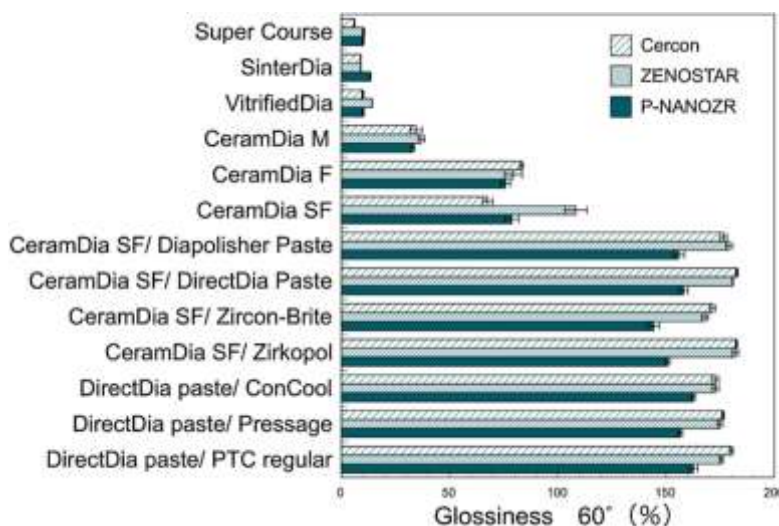


Fig 3: Glossiness of three types of dental zirconia finished with 13 types of grinding and polishing condition.

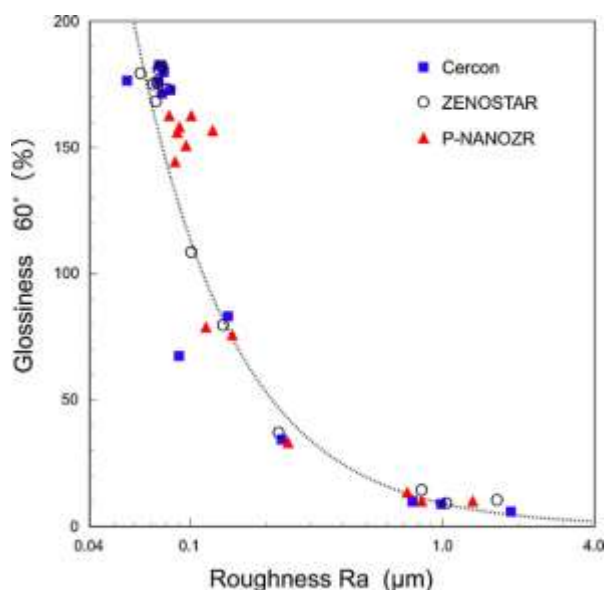


Fig. 4. Relation between surface roughness and glossiness of three types of dental zirconia finished with 13 types of grinding and polishing condition.

The amount of wear on restorative materials depends on their structure and particle size. Zirconia, which has a consistent structure, can be polished to a mirror finish with the right tools and materials. There is no need to worry about enamel wear when zirconia restorations are used. However, if the surface of the zirconia is rough, it can cause significant wear on opposing enamel. Therefore, it is important to polish the surface of zirconia restorations when making occlusal adjustments, and glazing is not recommended for finishing the surface.

7. Evaluation of clinical efficacy on zirconia restoration.

CAD/CAM-produced Y-TZP-based systems are in considerable demand in esthetic and stress-bearing regions. The highly esthetic nature of zirconia with its superior physical properties and biocompatibility makes it an effective restorative system to meet the demands of modern patients [46-48]. Currently, endowing a removable knob to the dental prosthesis apparatus has made it possible to treat temporary cementation which means temporary crowns are usually made of acrylic or composite and cemented with zinc oxide eugenol/non eugenol cements. Partially stabilized Zirconia is considered the top choice for all-ceramic restorations due to its excellent strength and fracture resistance, as supported by numerous research studies since the late 1990s[49]. In order to benefit from the strength of the core material, the bond between the core and veneer must be strong enough to handle the functional

stresses that the esthetic veneer puts on it. CAD/CAM-produced zirconia was introduced in Japan in 2005. Several clinical studies have found that porcelain veneers on posterior zirconia-based ceramic restorations often chip or fracture at a higher rate.

II. CONCLUSION:

Y-TZP, a type of dental material, has strong mechanical properties and is resistant to fractures, but it lacks translucency. To address this, porcelain is often layered onto the Y-TZP framework. Recent advancements in scanning, CAD software, networked machining centers, and other dental CAD/CAM technologies have made it easier to fabricate Y-TZP frameworks with a good fit. This has made zirconia-based fixed partial dentures (FPDs) more promising. However, dentists and dental technicians still need to collaborate and follow proper clinical procedures, even with the help of CAD/CAM technology. Longer clinical evaluations are necessary to further prove the effectiveness of zirconia-based FPDs, especially with new options available.

REFERENCES

- [1]. Guazzato M, Albakry M, Ringer SP, Swain MV. Strength, fracture toughness and microstructure of a selection of all-ceramic materials. Part II. Zirconia-based dental ceramics. *Dent Mater* 2004;20:449-56.
- [2]. Guazzato M, Proos K, Quach L, Swain MV. Strength, reliability and mode of



- fracture of bilatered porcelain/zirconia (Y-TZP) dental ceramics. *Biomaterials* 2004;25:5045-5052.
- [3]. Luthardt RG, Holzhter M, Sandkuhl O, Herold V, Schnapp JD, Kuhlisch E, Walter M. Reliability and properties of ground y-tzp-zirconia ceramics. *J Dent Res* 2002;81:487-491.
- [4]. Zhang Y, Lawn B, Rekow ED, Thompson VP. Effect of sandblasting on the long-term performance of dental ceramics. *J Biomed Mater Res B Appl Biomater* 2004;71:381-386.
- [5]. Zhang Y, Lawn B. Long-term strength of ceramics for biomedical applications. *J Biomed Mater Res B Appl Biomater* 2004;69:166-172.
- [6]. Piconi C, Maccauro G. Zirconia as a ceramic biomaterial. *Biomaterials* 1999;20:1-25.
- [7]. Subbarao EC. Zirconia-an overview. *The American Ceramic Society*; 1981. p. 1-24.
- [8]. Goff JP, Hayes W, Hull S, Hutchings MT, Clausen KN. Defect structure of yttria-stabilized zirconia and its influence on the ionic conductivity at elevated temperatures. *Phys Rev B* 1999;59:14202-19.
- [9]. Jeffrey Y, Thompson, Brian R, Stoner, Jeffrey R, Piascik, Robert Smith. Adhesion/cementation to zirconia and other non-silicate ceramics: Where are we now? *dental materials* 27 (2 0 1 1) 71-82.
- [10]. Keith O, Kusy RP, Whitley JQ. Zirconia brackets: an evaluation of morphology and coefficients of friction. *Am J Orthod Dentofacial Orthop* 1991;106:605-11.
- [11]. Koutayas SO, Kern M. All-ceramic posts and cores: the state of the art. *Quintessence Int* 1999;30:383-92.
- [12]. Meyenberg KH, Luthy H, Scharer P. Zirconia posts: a new all-ceramic concept for nonvital abutment teeth. *J Esthet Dent* 1995;7:73-80.
- [13]. Prestipino V, Ingber A. Esthetic high-strength implant abutments: Part 1. *J Esthet Dent* 1993;5:29-36.
- [14]. Yildirim M, Edelhoff D, Hanisch O, Spiekermann H. Ceramic abutments—a new era in achieving optimal esthetics in implant dentistry. *Int J Periodontics Restorative Dent* 2000;20:81-91.
- [15]. Potiket N, Chiche G, Finger IM. In vitro fracture strength of teeth restored with different all-ceramic crown systems. *J Prosthet Dent* 2004;92:491-5.
- [16]. Tinschert J, Natt G, Mautsch W, Augthun M, Spiekermann H. Fracture resistance of lithium disilicate-, alumina-, and zirconia-based three-unit fixed partial dentures: a laboratory study. *Int J Prosthodont* 2001;14:231-8.
- [17]. Valandro LF, Mallmann A, Kella Bona A, Bottino MA. Bonding to densely sintered and glass infiltrated aluminum and zirconium-based ceramics. *J Appl Oral Sci* 2005;13:47-52.
- [18]. Valandro LF, Özcan M, Bottino MA, Bottina MC, Scotti R, Della Bona A. Bond strength of a resin cement to high-alumina and zirconia-reinforced ceramics: the effect of surface conditioning. *J Adhes Dent* 2006;8:175-81.
- [19]. Wegner SM, Kern M. Long-term resin bond strength to zirconia ceramic. *J Adhes Dent* 2000;2:139-47.
- [20]. Derand P, Derand T. Bond strength of luting cements to zirconium oxide ceramics. *Int J Prosthodont* 2000;13:131-5.
- [21]. Guazzato M, Quach L, Albakry M, Swain MV. Influence of surface and heat treatments on the flexural strength of Y-TZP dental ceramic. *J Dent*. 2005; 33(1):9-18.
- [22]. Zhang Y, Lawn BR, Rekow ED, Thompson VP. Effect of sandblasting on the long-term performance of dental ceramics. *J Biomed Mater Res B Appl Biomater*. 2004; 71(2):381-6.
- [23]. Guess PC, Zhang Y, Kim JW, Rekow ED, Thompson VP. Damage and reliability of Y-TZP after cementation surface treatment. *J Dent Res*. 2010; 89(6):592-6.
- [24]. Janda R, Roulet JF, Wulf M, Tiller HJ. A new adhesive technology for all-ceramics. *Dent Mater* 2003;19:567-73.
- [25]. Denry I, Kelly JR. State of the art of zirconia for dental applications. *Dent Mater* 2008;24:299-307.
- [26]. Eisenburger M, Mache T, Borchers L, Stiesch M. Fracture stability of anterior zirconia crowns with different core designs and veneered using the layering or the press-over technique. *Eur J Oral Sci* 2011;119:253-7.
- [27]. Guess PC, Bonfante EA, Silva NR, Coelho PG, Thompson VP. Effect of core design and veneering technique on damage and reliability of Y-TZP supported crowns. *Dent Mater* 2013;29:307-16.



- [28]. Preis V, Letsch C, Handel G, Behr M, Schneider-Feyrer S, Rosentritt M. Influence of substructure design, veneer application technique, and firing regime on the in vitro performance of molar zirconia crowns. *Dent Mater* 2013;29:e113–21.
- [29]. Fischer J, Grohmann P, Stawarczyk B. Effect of zirconia surface treatments on the shear strength of zirconia/veneering ceramic composites. *Dent Mater J* 2008;27:448–54.
- [30]. ISO 9693. Metal-ceramic dental restorative systems. Geneva: International Organization for Standardization; 1999.
- [31]. Doi M, Yoshida K, Atsuta M, Sawase T. Influence of pre-treatments on flexural strength of zirconia and debonding crack-initiation strength of veneered zirconia. *J Adhes Dent* 2011;13:79–84.
- [32]. Tada K, Sato T, Yoshinari M. Influence of surface treatment on bond strength of veneering ceramics fused to zirconia. *Dent Mater J* 2012;31: 287–96.
- [33]. Yamaguchi H, Ino S, Hamano N, Okada S, Teranaka T. Examination of bond strength and mechanical properties of Y-TZP zirconia ceramics with different surface modifications. *Dent Mater J* 2012;31:472–80.
- [34]. Kern M, Thompson VP. Bonding to a glass infiltrated alumina ceramic: adhesion methods and their durability. *J Prosthet Dent* 1995;73:240–9.
- [35]. Kern M, Wegner SM. Bonding to zirconia ceramic: adhesion methods and their durability. *Dent Mater* 1998;14:64–71.
- [36]. Janda R, Roulet JF, Wulf M, Tiller HJ. A new adhesive technology for allceramics. *Dent Mater* 2003;19:567–73.
- [37]. Blatz MB, Sadan A, Martin J, Lang B. In vitro evaluation of shear bond strengths of resin to densely-sintered high-purity zirconium-oxide ceramic after long-term storage and thermal cycling. *J Prosthet Dent* 2004;91:356–62.
- [38]. Atsu SS, Kilicarslan MA, Kucukesmen HC, Aka PS. Effect of zirconiumoxide ceramic surface treatments on the bond strength to adhesive resin. *J Prosthet Dent* 2006;95:430–6.
- [39]. Blatz MB, Chiche G, Holst S, Sadan A. Influence of surface treatment and simulated aging on bond strengths of luting agents to zirconia. *Quintessence Int* 2007;38:745–53.
- [40]. Tanaka R, Fujishima A, Shibata Y, Manabe A, Miyazaki T. Cooperation of phosphate monomer and silica modification on zirconia. *J Dent Res* 2008;87:666–70.
- [41]. 3M ESPE Lava crowns and bridges (7 years). *The Dental Advisor* 2010;27(7). available at: <http://www.dentaladvisor.com/clinical-evaluations/evaluations/3m-espe-lava-crownsand-bridges-7-yr.shtml> [Last accessed September 5, 2013].
- [42]. Bona AD, Kelly JR. The clinical success of all-ceramic restorations. *J Am Dent Assoc* 2008;139(Suppl. 4):8S–13S.
- [43]. Baldissara P, Llukacej A, Ciocca L, Valandro FL, Scotti R. Translucency of zirconia copings made with different CAD/CAM systems. *J Prosthet Dent* 2010;104:6–12.
- [44]. Alghazzawi TF, Lemons J, Liu PR, Essig ME, Janowski GM. Evaluation of the optical properties of CAD-CAM generated yttria-stabilized zirconia and glass-ceramic laminate veneers. *J Prosthet Dent* 2012;107:300–8.
- [45]. Ban S. Polishing of zirconia full contour restoratives and antagonist wear. *QDT* 2012;32:1240–54 (In Japanese).
- [46]. Vult von Steyern P, Ebbesson S, Holmgren J, Haag P, Nilner K. Fracture strength of two oxide ceramic crown systems after cyclic pre-loading and thermocycling. *J Oral Rehabil* 2006;33:682–9.
- [47]. Fritzsche J. Zirconium oxide restorations with the DCS precidentsystem. *Int J Comput Dent* 2003;6:193–201.
- [48]. Paolo V, Mutinelli S. Evaluation of zirconium-oxide-based ceramic single-unit posteriorfixed dental prostheses (FDPs) generated with two CAD/CAM systems compared to porcelain-fused-to-metal single-unit posterior FDPs: A 5-year clinical prospective study. *J Prosthodont* 2012;21:265–9.
- [49]. Tinschert J, Zweg D, Marx R, Anusavice KJ. Structural reliability of alumina-, feldspar-, leucite-, mica- and zirconia-based ceramics. *J Dent* 2000;28:529–35.
- [50]. Takashi Miyazaki , Takashi Nakamura, Hideo Matsumura , Seiji Ban , Taira Kobayashi. Current status of zirconia restoration. *Journal of Prosthodontic Research* 57 (2013) 236–261